


Data file: D:\CHEM32\1\DATA\M10196Final.D
 Sample name: M10196-RADA16-03
 Description: Mobile Phase: Buffer A: 0.1% TFA in H2O
 Buffer B: 0.1% TFA in ACN
 Gradient: 9-19%B in 20min, Flow rate: 1.0ml/min
 Column: Unitary C18 5um 100A 4.6*150mm
 Instrument: Agilent HPLC 1100

Instrument: 1100

Location: 53
 Injection: 1 of 1
 Injection volume: 10.000
 Acq. operator: SYSTEM

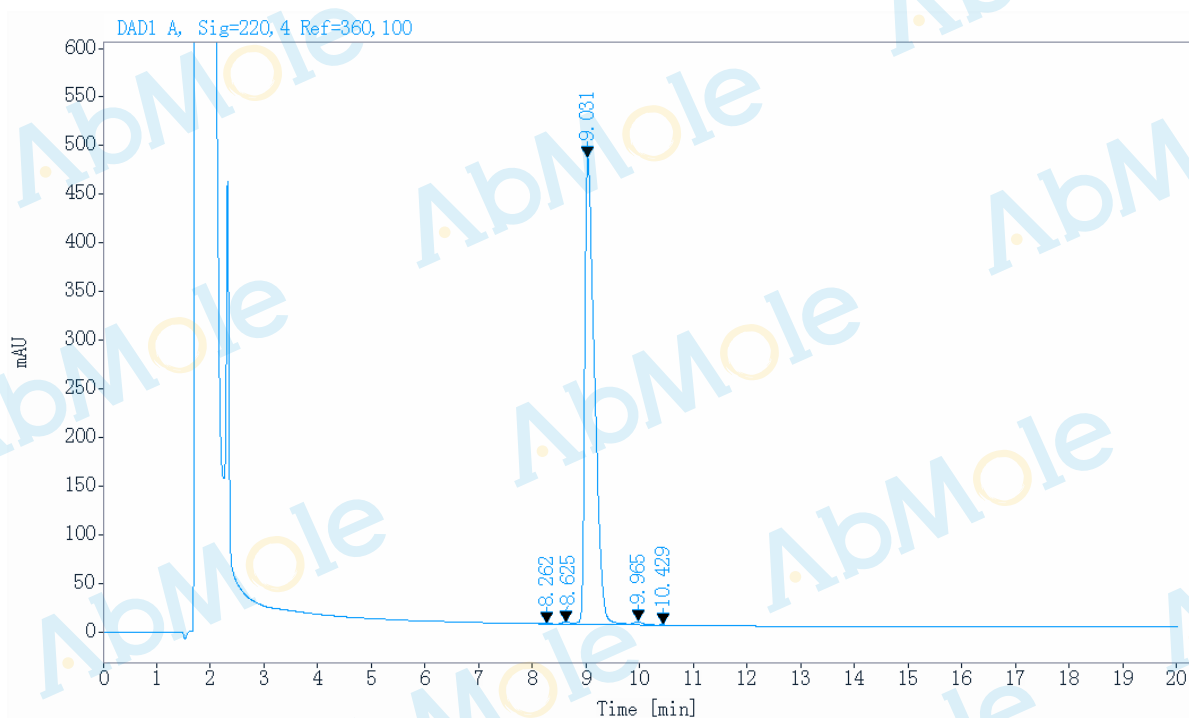

Signal: DAD1 A, Sig=220, 4 Ref=360, 100

RT[mi n]	Type	Width[mi n]	Area	Height	Area% Name
8.262	MM	0.3617	24.5383	1.1307	0.3956
8.625	MF	0.1786	28.5641	2.6655	0.4606
9.031	FM	0.2115	6092.8394	480.2375	98.2380
9.965	MF	0.2141	46.4945	3.6192	0.7497
10.429	FM	0.3631	9.6817	0.4444	0.1561
	Sum		6202.1179		