


SAMPLE INFORMATION

Sample Name:	M1966-Fulvestrant-08	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	M1966
Vial:	58	Acq. Method Set:	CD_05_95_15min_40D
Injection #:	1	Processing Method:	LC PQ
Injection Volume:	5.00 ul	Channel Name:	220.0nm
Run Time:	15.0 Minutes	Proc. Chnl. Descr.:	W2996 PDA 220.0 nm (PDA)

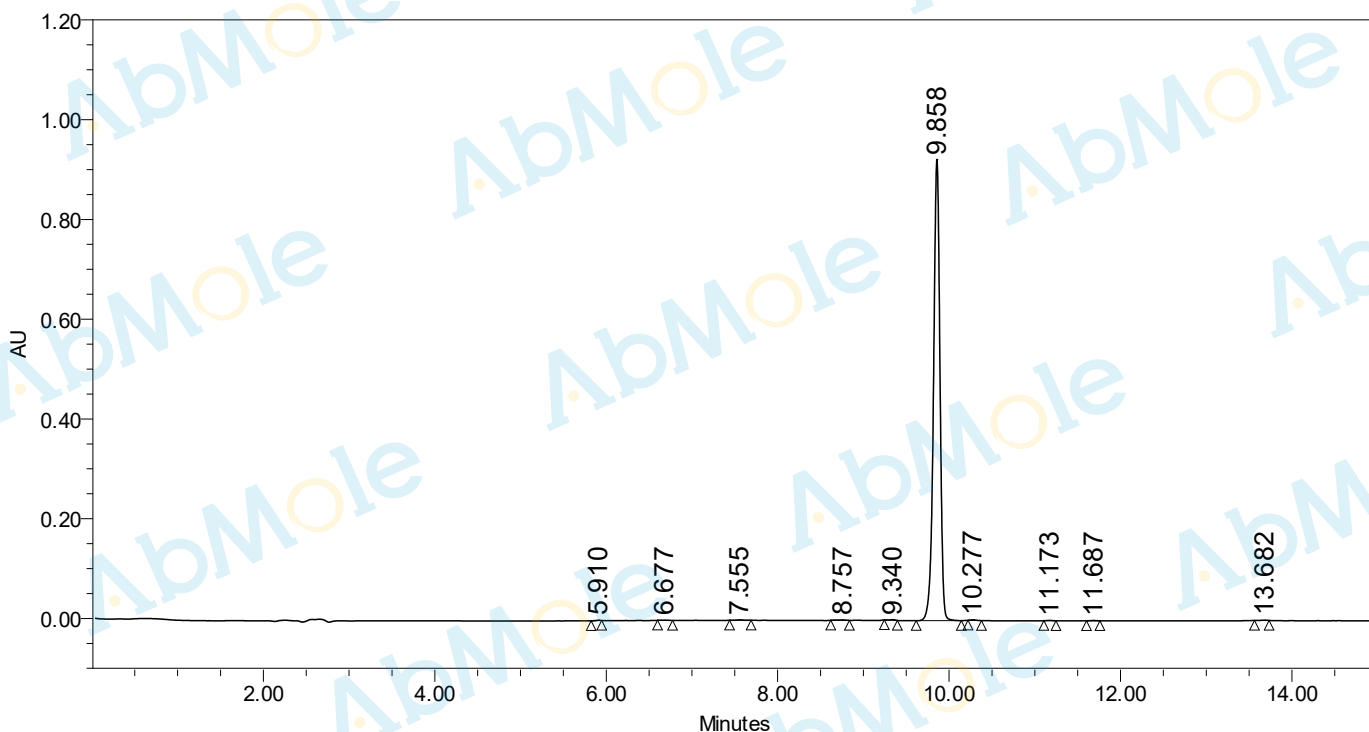

	RT	Area	% Area	Height
1	5.910	1958	0.04	611
2	6.677	1382	0.03	241
3	7.555	4299	0.09	884
4	8.757	6240	0.13	777
5	9.340	4291	0.09	1081
6	9.858	4818719	99.35	925547
7	10.277	5351	0.11	1184

	RT	Area	% Area	Height
8	11.173	2911	0.06	681
9	11.687	2915	0.06	593
10	13.682	2351	0.05	431