


SAMPLE INFORMATION

Sample Name:	M2320-17-AAG-07	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	M2320
Vial:	66	Acq. Method Set:	CD_05_95_15min_40D
Injection #:	1	Processing Method:	LC PQ
Injection Volume:	12.00 ul	Channel Name:	240.0nm
Run Time:	15.0 Minutes	Proc. Chnl. Descr.:	W2996 PDA 240.0 nm (PDA)

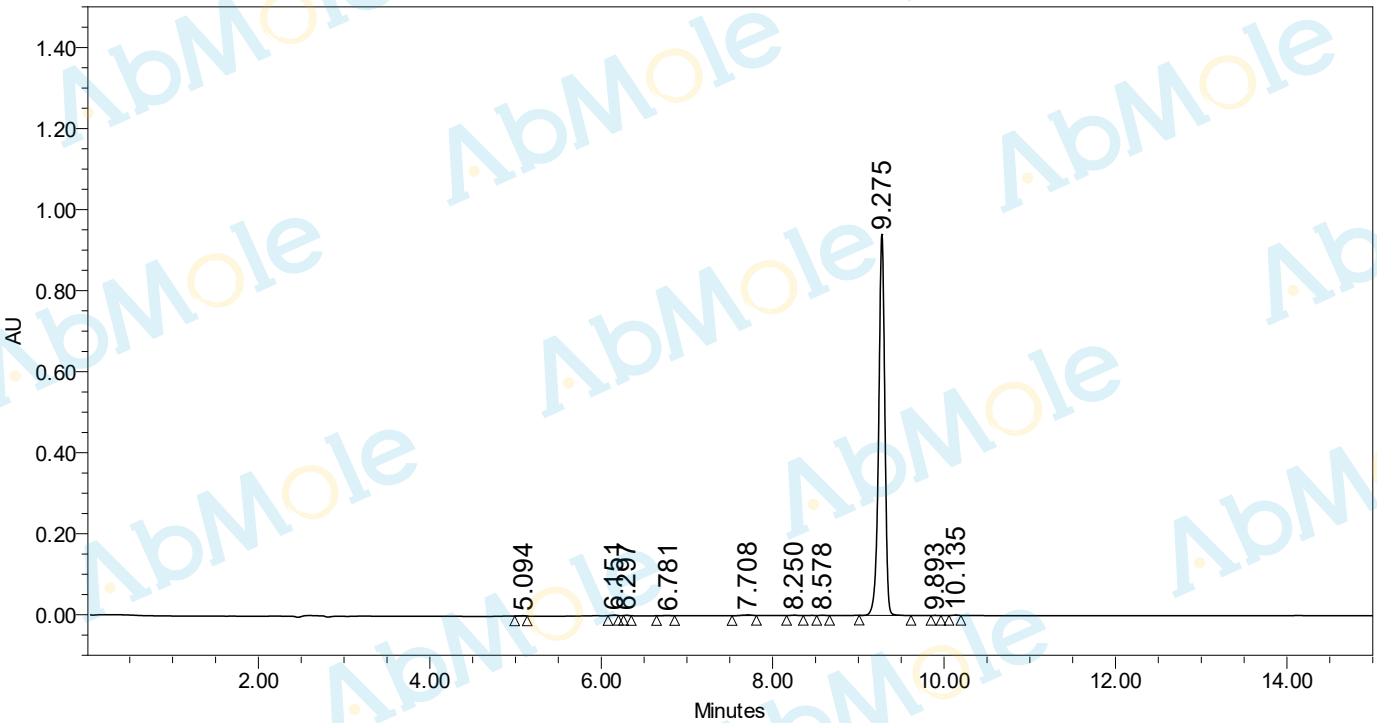

	RT	Area	% Area	Height
1	5.094	3712	0.08	846
2	6.151	4359	0.09	977
3	6.297	1996	0.04	627
4	6.781	3097	0.07	389
5	7.708	11582	0.24	1471
6	8.250	3939	0.08	854
7	8.578	2334	0.05	563

	RT	Area	% Area	Height
8	9.275	4715979	99.25	941409
9	9.893	827	0.02	255
10	10.135	3621	0.08	813