


MASS SPECTROMETRY REPORT

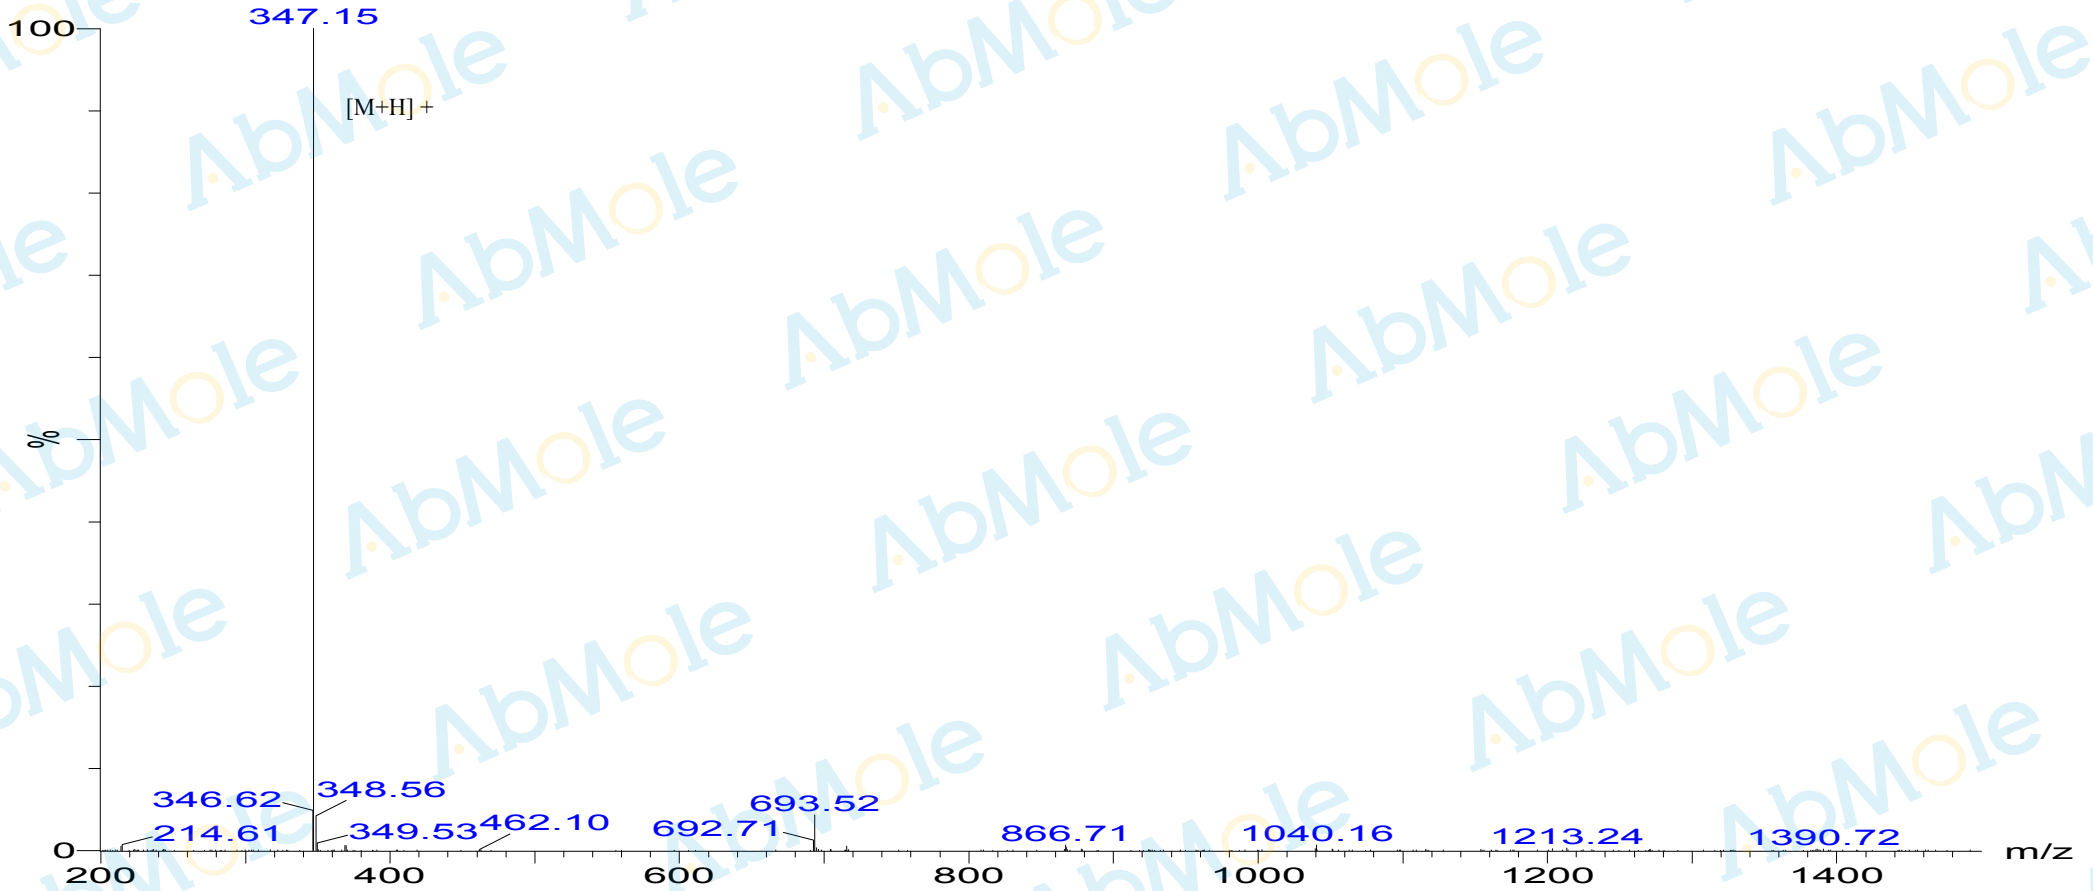

Sample Description

Analyst: SHAO
Sample: M2976-RGD-04
M.W.: 346.3
Lot. No.:

Instrument

Probe:
Nebulizer Gas Flow:
CDL:
CDL Temp.:
Block Temp.:

Waters 2695

ESI
1.5L/min
-20.0v
250 °C
200 °C

Probe Bias:

Detector:

T. Flow:

B. Conc.:

+4.5kv

1.5kv

0.5ml/min

50%H2O/50%ACN