


SAMPLE INFORMATION

Sample Name:	M3006-Sertraline hydrochloride-02	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	20251231
Vial:	1	Acq. Method Set:	CD_05_95_15min_40D
Injection #:	1	Processing Method:	LC PQ
Injection Volume:	6.00 ul	Channel Name:	220.0nm
Run Time:	15.0 Minutes	Proc. Chnl. Descr.:	W2996 PDA 220.0 nm (PDA)

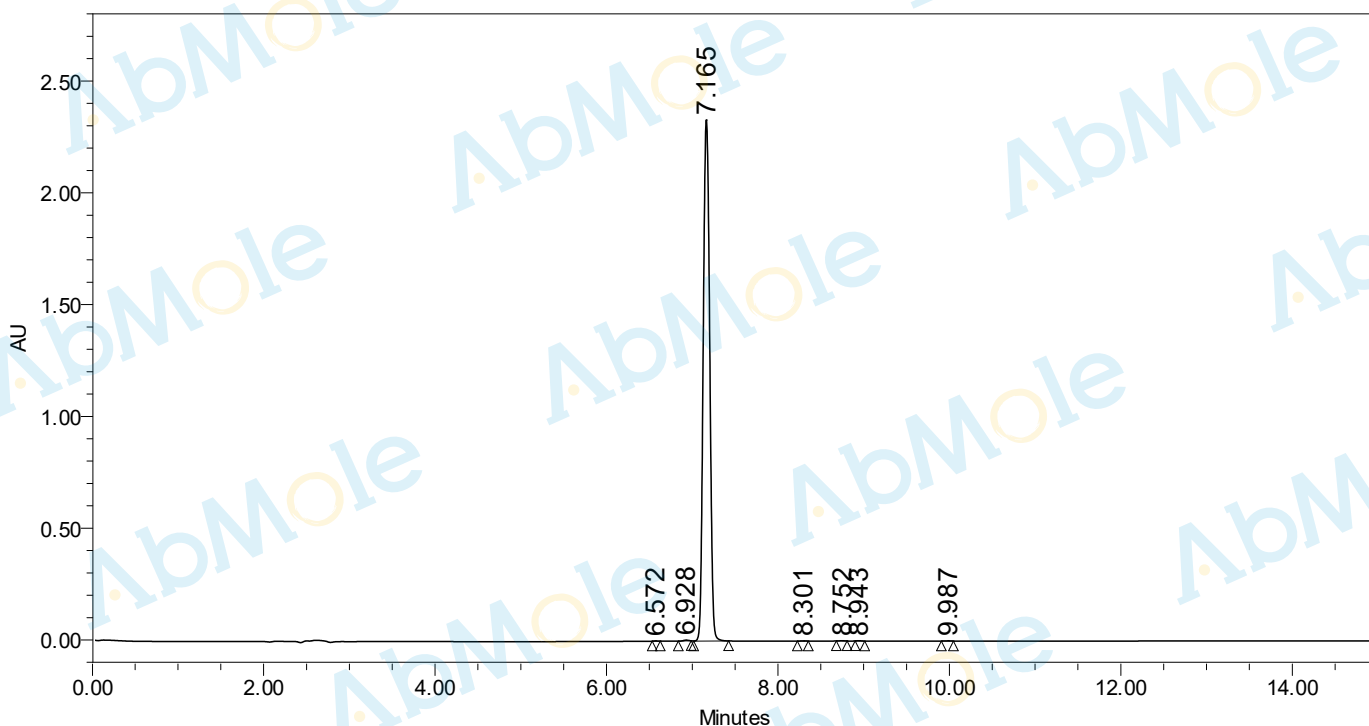

	RT	Area	% Area	Height
1	6.572	2570	0.02	831
2	6.928	13580	0.11	3346
3	7.165	12249782	99.74	2332311
4	8.301	3476	0.03	882
5	8.752	3705	0.03	791
6	8.943	4002	0.03	1096
7	9.987	4372	0.04	965