


Data file: D:\CHEM32\1\DATA\M31233-03Final.D  
 Sample name: M31233- $\omega$ -Agatoxin IVA-03  
 Description: Mobile Phase: Buffer A: 0.1% TFA in H2O  
 Buffer B: 0.1% TFA in ACN  
 Gradient: 27-37%B in 20min, Flow rate: 1.0ml/min  
 Column: Unitary C18 5um 100A 4.6\*150mm  
 Instrument: Agilent HPLC 1100

Instrument: 1100  
 Location: 3  
 Injection: 1 of 1  
 Injection volume: 10.000  
 Acq. operator: SYSTEM

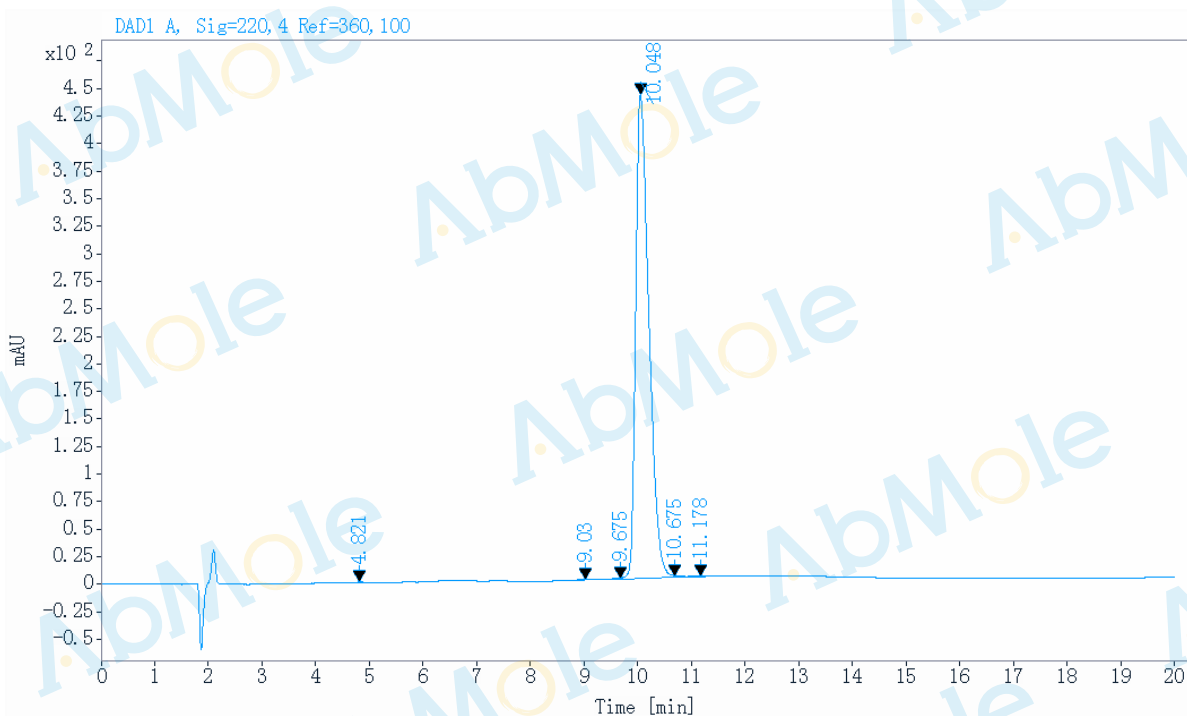

Signal: DAD1 A, Sig=220, 4 Ref=360, 100

RT[mi n]	Type	Width[mi n]	Area	Height	Area% Name
4.821	MM	0.1756	7.5165	0.7133	0.0992
9.030	MF	0.2447	12.5895	0.8573	0.1661
9.675	MF	0.1736	9.5580	0.9177	0.1261
10.048	MF	0.2851	7510.1831	439.0489	99.1010
10.675	MF	0.1004	14.0517	1.6775	0.1854
11.178	FM	0.3890	24.4129	1.0458	0.3221
	Sum		7578.3117		