


Sample name: M40707-Icetrokinra-02
Description: Mobile Phase: Buffer A: 0.1% TFA in H2O
 Buffer B: 0.1% TFA in ACN
 Gradient: 27-37%B in 20min, Flow rate: 1.0ml/min
 Column: Unitary C18 5um 100A 4.6*150mm
 Instrument: Agilent HPLC 1100

Instrument: 1100
Location: 22
Injection: 1 of 1
Injection volume: 5.000
Acq. operator: System

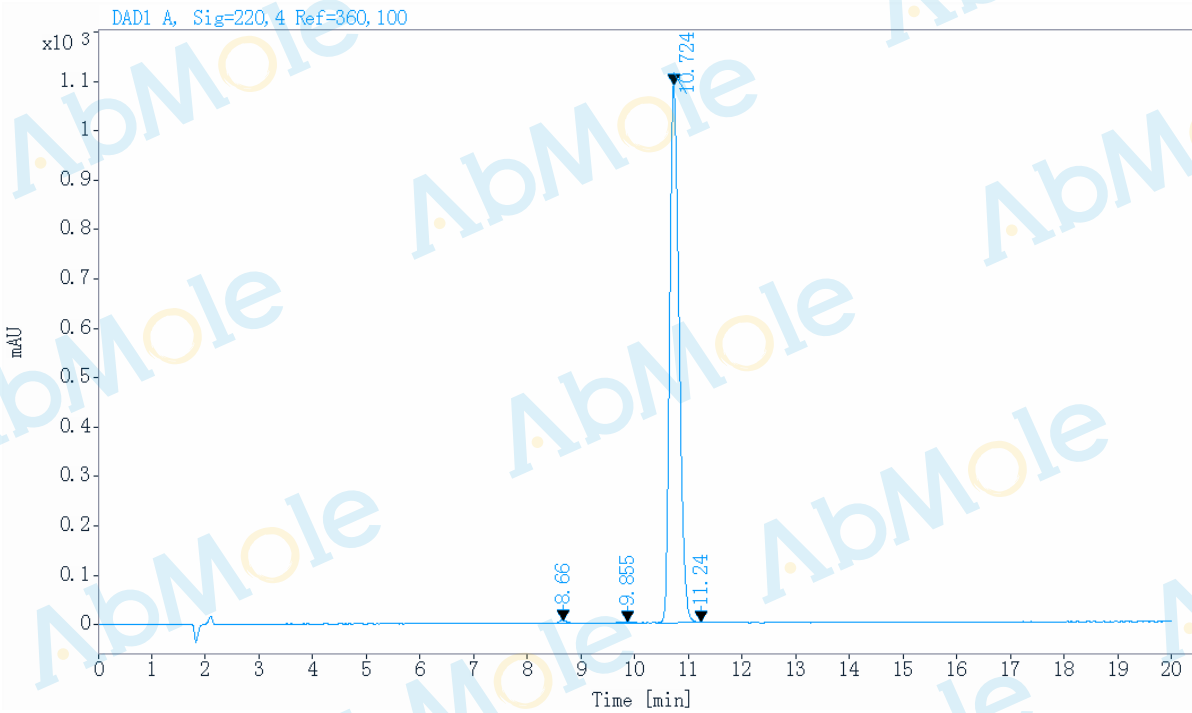

Signal: DAD1 A, Sig=220, 4 Ref=360, 100

RT[mi n]	Type	Width[mi n]	Area	Height	Area% Name
8.660	BB	0.1769	64.5817	5.8467	0.4847
9.855	MM	0.2077	27.2984	2.1908	0.2049
10.724	MF	0.2010	13220.9199	1096.2338	99.2219
11.240	FM	0.1325	11.8047	1.4847	0.0886
Sum			13324.6047		