


MASS SPECTROMETRY REPORT

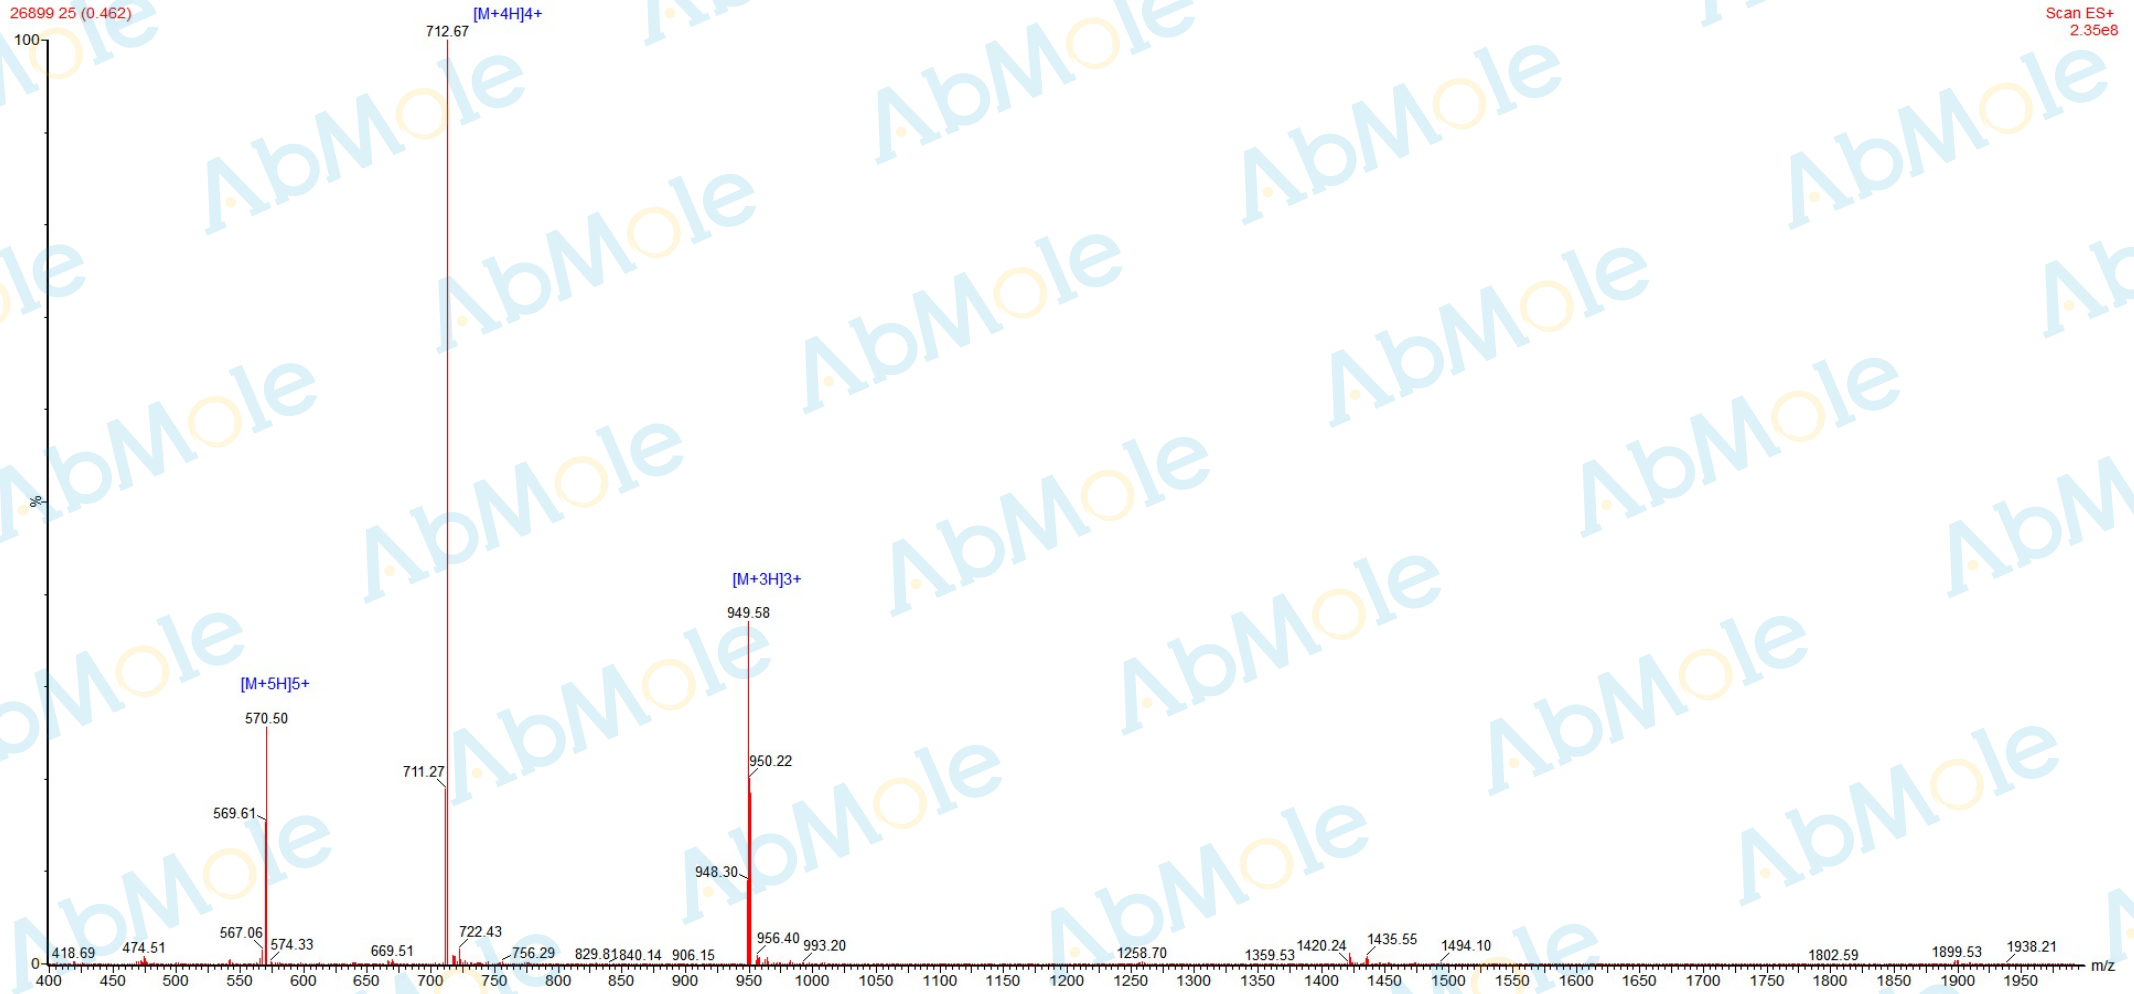

Sample Description

Analyzed date: 2026-01-20
Analyst: PY
Sample: M49432-Melittin-03
M.W.: 2846.50
Lot. No.: 202603

Instrument

Probe:
Nebulizer Gas Flow:
CDL:
CDL Temp.:
Block Temp.:

Waters ZQ2000

ESI
-20.0v
250 °C
200 °C
Probe Bias: +4.5kv
Detector: 1.5kv
T. Flow: 0.2ml/min
B. Conc.: 50%H2O/50%ACN