


MASS SPECTROMETRY REPORT

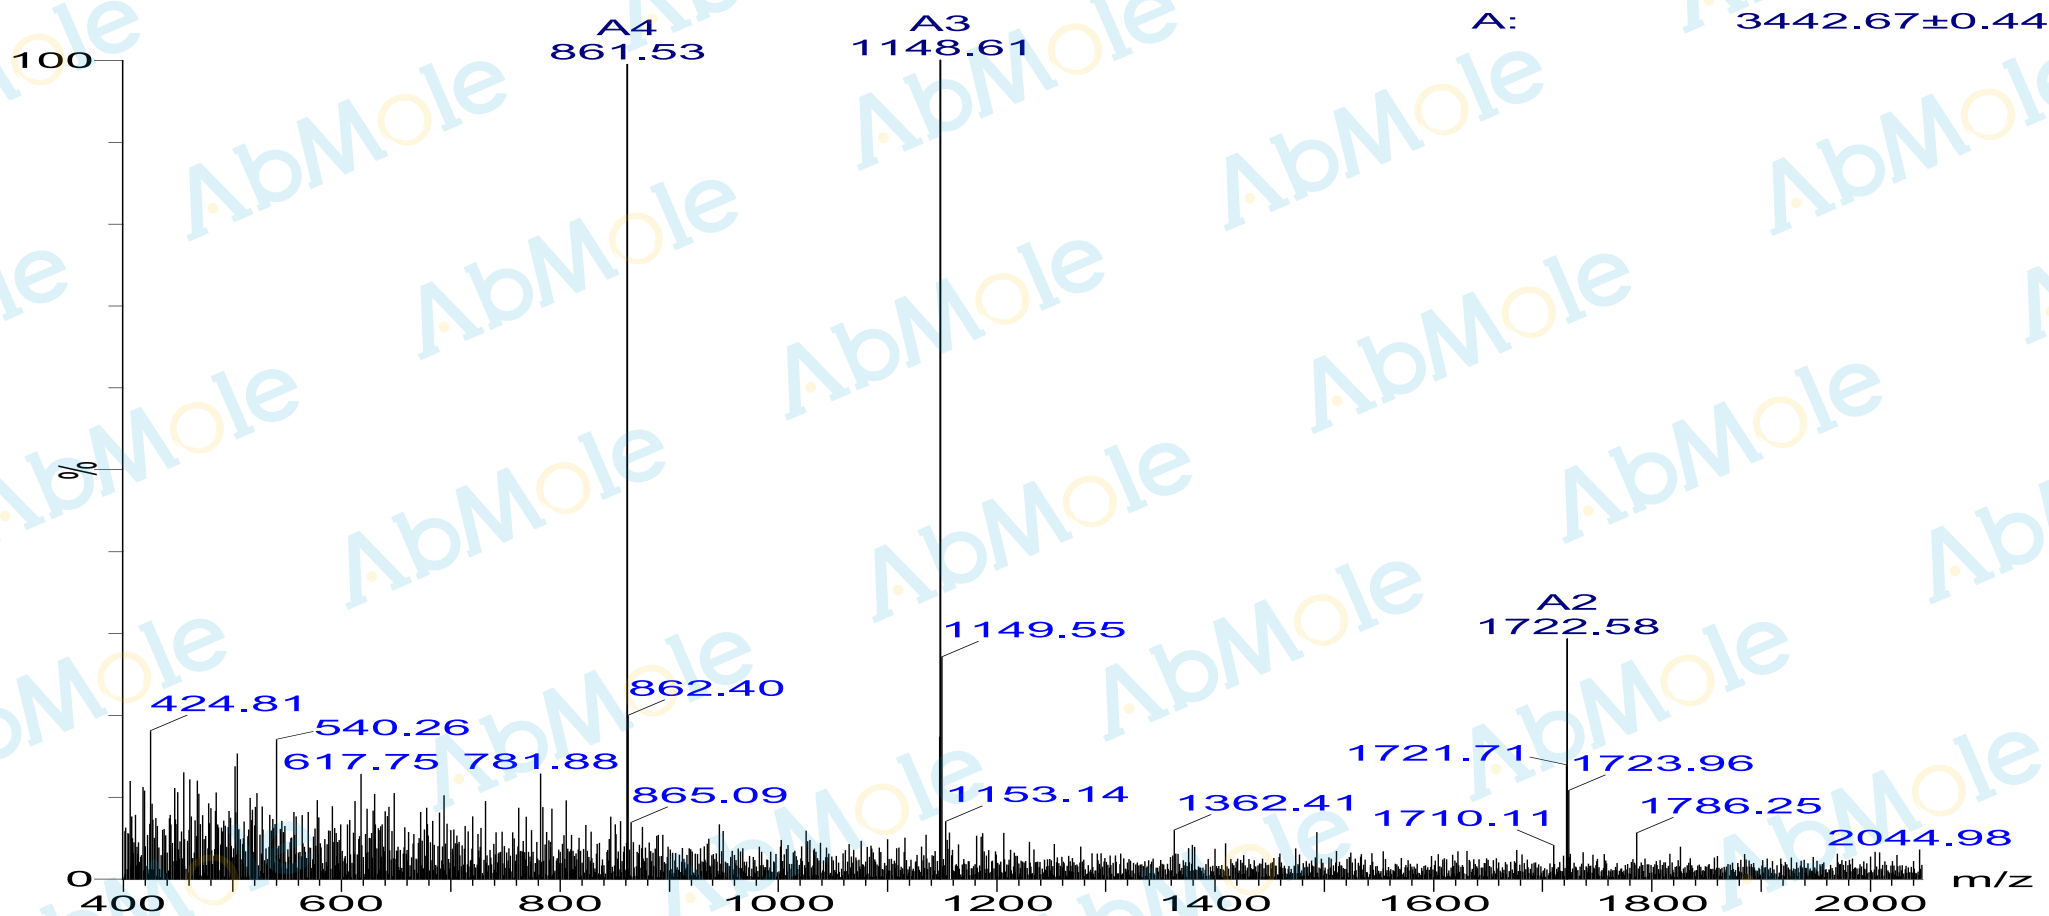

Sample Description

Analyst: SHAO
 Sample: M53664-Defensin HNP-1 human TFA-02
 M.W.: 3442.1
 Lot. No.:

Instrument

Waters ZQ 2000
 Probe: ESI
 Desolvation Gas Flow: 250L/Hr
 Cone: 35.0V
 Desolvation Temp.: 200 °C
 Source Temp.: 120 °C

Capillary: 3.0kV
 Extractor: 3.0V
 RF Lens: 0.1V
 T. Flow: 0.5ml/min
 B. Conc.: 50%H2O/50%ACN